
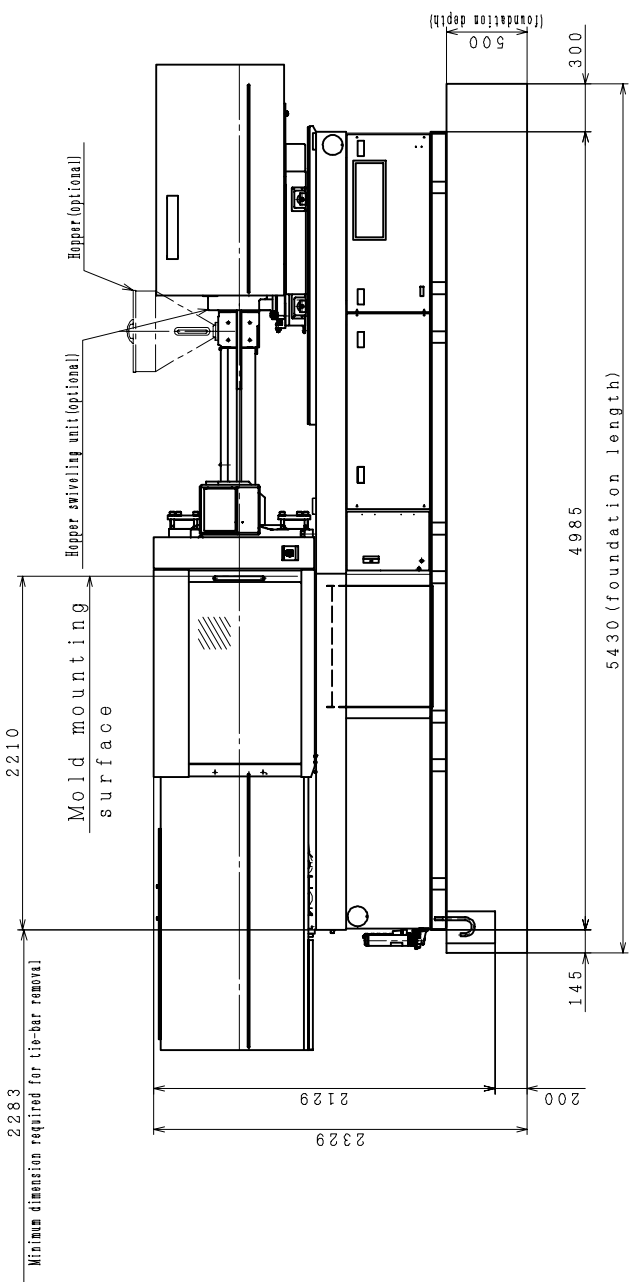
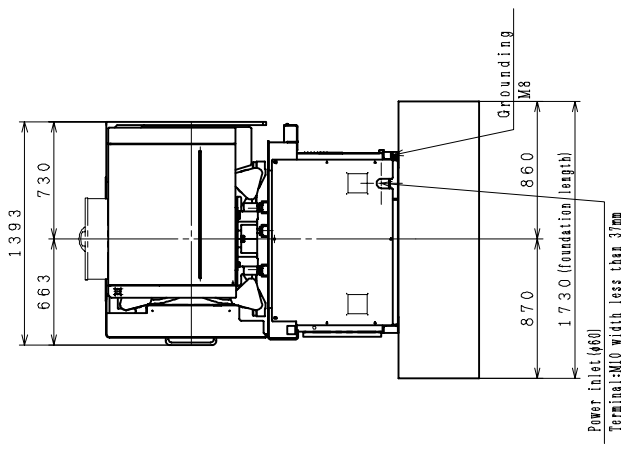


<Note>

- 1) Detail information about foundation is available upon request, if any.
- 2) The primary piping of cooling water should be made using flexible piping such as a rubber hose. And also, the inlet wiring of power source should be made using flexible cable such as a rubber sheath cord.

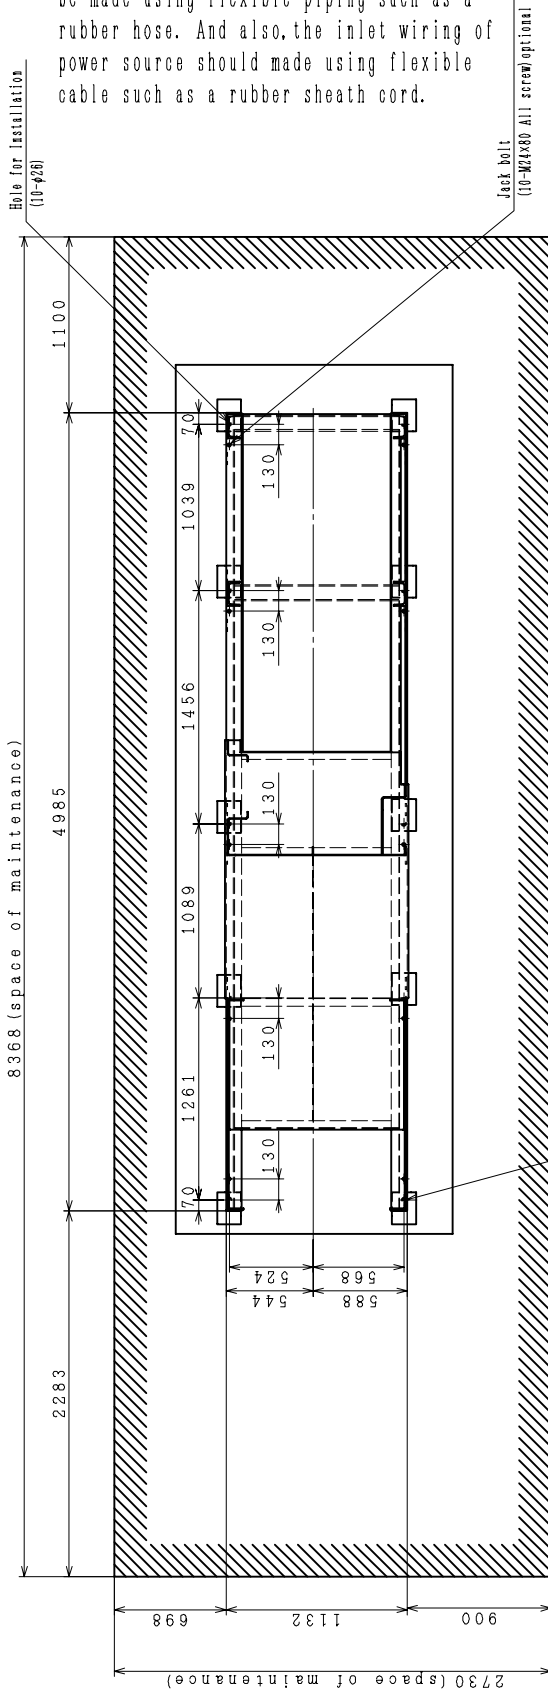

T49306

10-900

230MEt III (CE)

FOUNDATION DRAWING